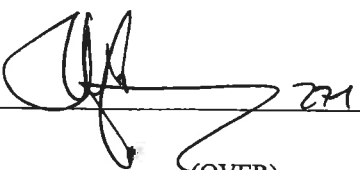


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	(30130) ✓
Name	Jeremy C. Kling	ID#	6715 ✓
Date	10.26.10 ✓		
A	Agency	VPD	Phone # 835-4560
	Instrument Location	VPD Jail	
B	Alco S/N	X172988 ✓	Target Value
			-085 ✓
			High Pressure
			250
	Alco Test Value Average	.084 ✓	.083 ✓
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
	Signature	 (OVER)	


8mm  
12/9/10


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (Do Not write in the area below)
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
  - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
  - (3) I am the Scientific Director of the State Breath Alcohol Program.
  - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
  - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
  - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 22<sup>nd</sup> day of DEC, 2010.

  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130130

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130130

OCTOBER 26, 2010

OPERATOR'S NAME:  
CONKLING/JEREMY/WHEELER  
OPERATOR'S NUMBER: 6715  
SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/NI :  
VOC

O.L. #: VOC

DEPT/AGENCY: UDZ1

CASE/REPORT: VOC

TEST TYPE: U

ALCO TARGET VALUE: .085

ALCO S/N: X172988

--- BREATH ANALYSIS ---

.085 ADJUSTED FOR 29.88 in  
ALCO TARGET .084 00:22  
BLANK TEST .000 00:23  
INTERNAL STANDARD VERIFIED 00:23  
ALCO TV 29.88 in .084 00:23  
BLANK TEST .000 00:24  
SUBJECT SAMPLE .000 00:25  
BLANK TEST .000 00:25  
ALCO TV 29.90 in .083 00:26  
BLANK TEST .000 00:27

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130130

OCTOBER 26, 2010  
TIME 08:20

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 40c

BAROMETER: 29.88 in

FLOW DETECTOR: OKAY

PUMP  
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST  
!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF  
GHIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~  
printtest()